


biolitec® in Urology

TWISTER, XCAVATOR®

Minimally invasive laser therapy of BPH, tumors, condylomas, strictures and more

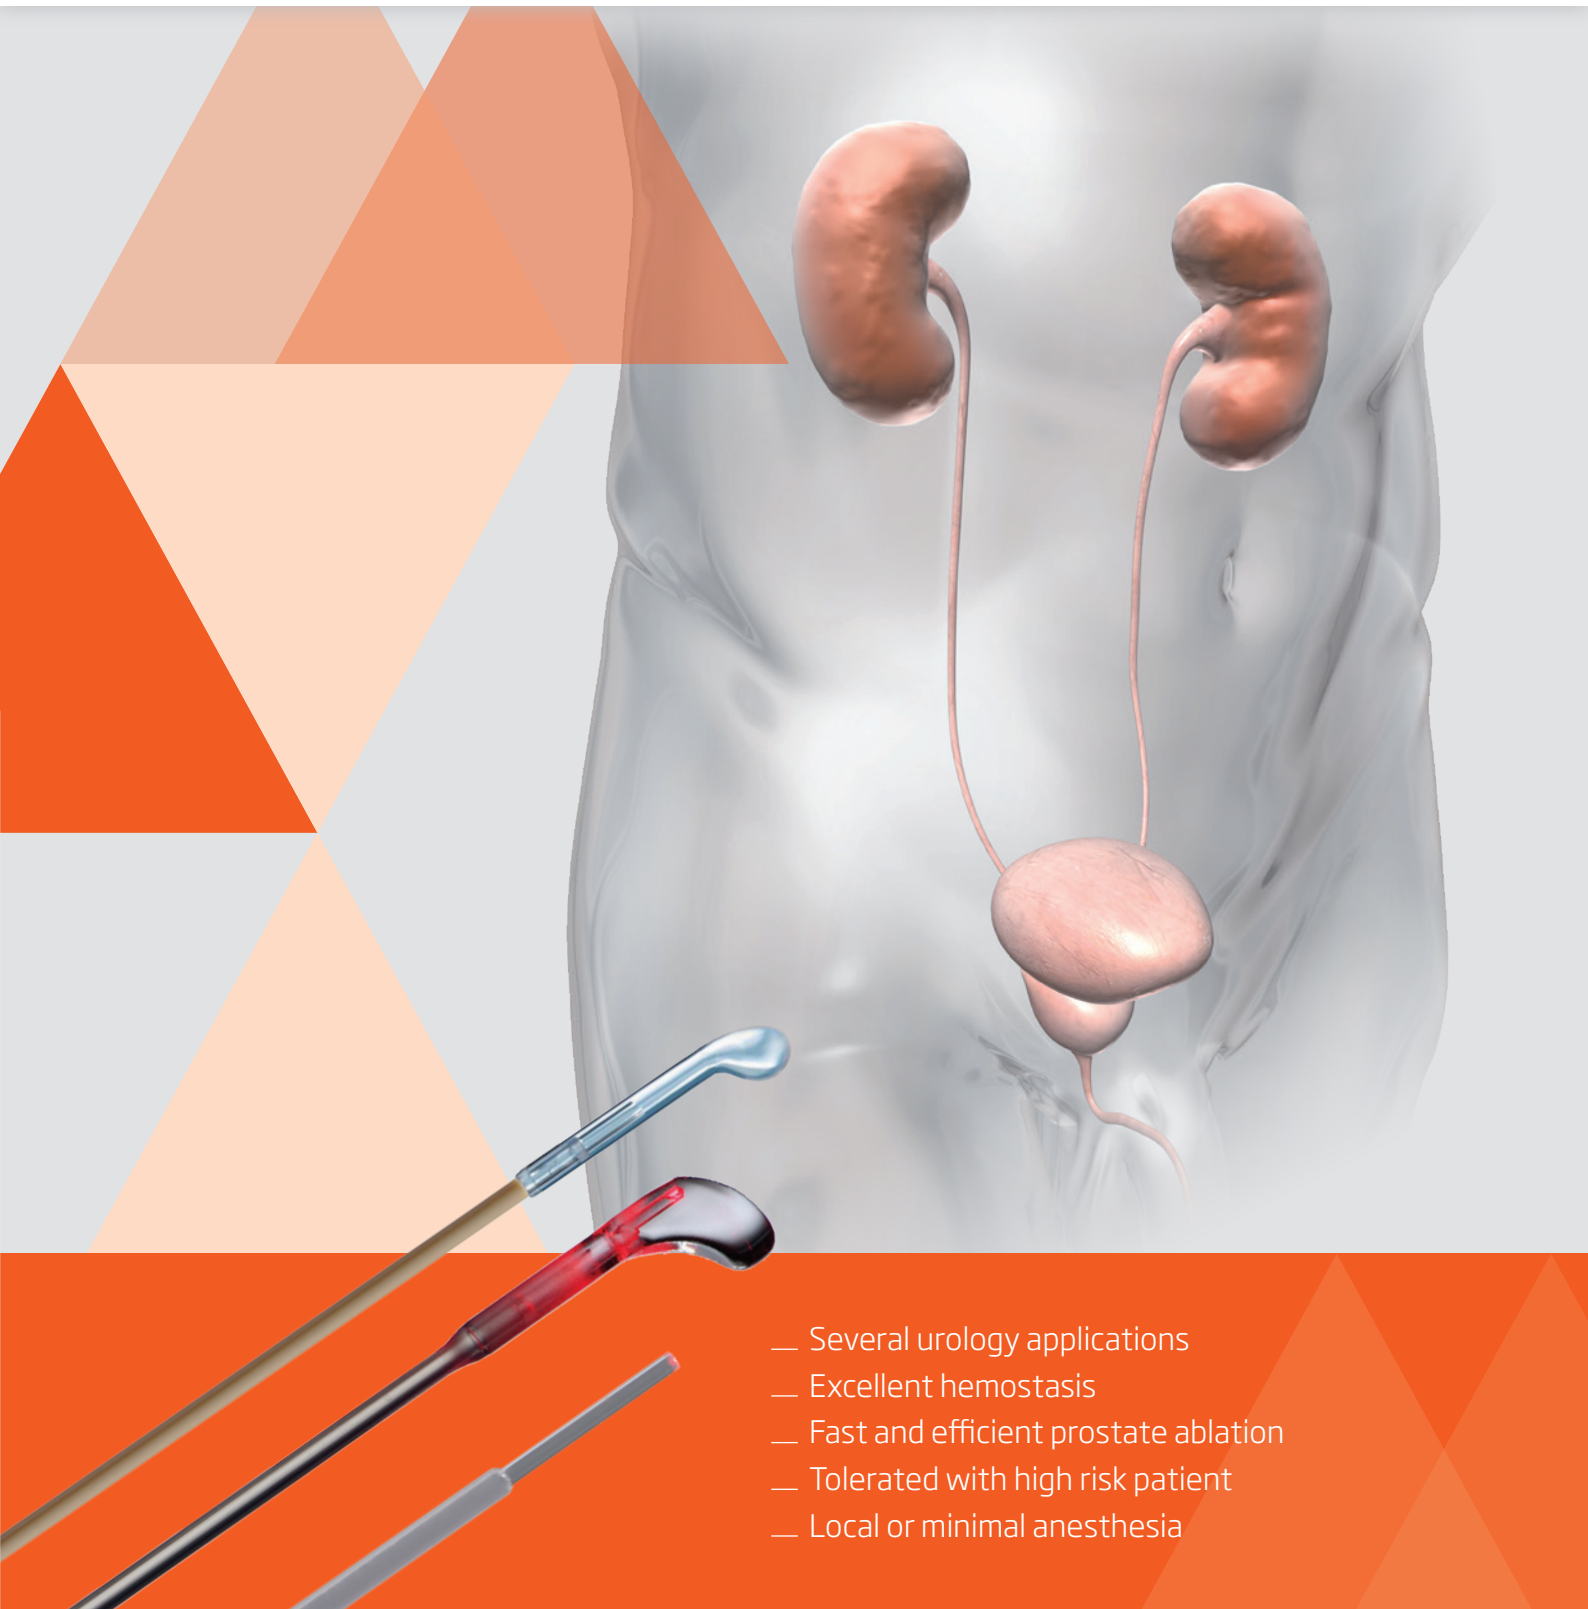



- Several urology applications
- Excellent hemostasis
- Fast and efficient prostate ablation
- Tolerated with high risk patient
- Local or minimal anesthesia

BPH – Benigne Prostatic Hyperplasia

Contact fiber approach with the XCAVATOR® and the TWISTER fibers

Our contact fibers are developed to reach out for unmatched ablation rates and excellent reliability. Working in contact mode offers direct and high energy delivery exact on the area where you want to ablate or vaporize. The results are smooth intrasurgical surfaces. Special developed glass tips assure working without fiber degradation and consistently high performance. More fiber control through tactile feedback shows the best outcome and permits outstanding treatment.



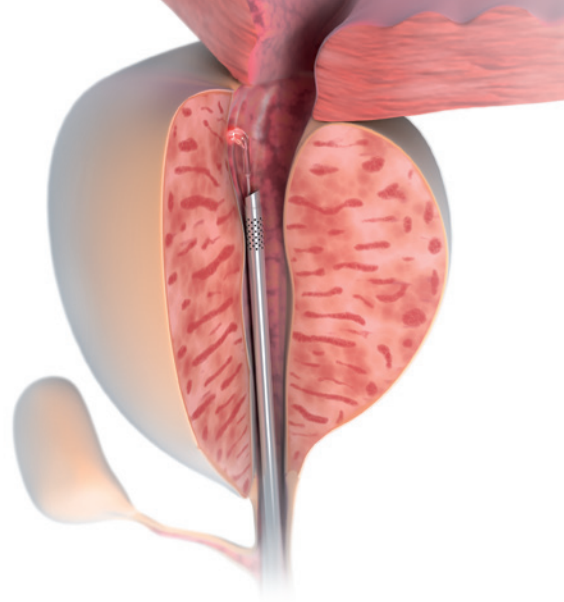

XCAVATOR®

Time is precious, so we designed the XCAVATOR® as the first true Laser-TURP to combine the efficacy of trans-urethral resection with the unmatched safety and hemostasis of the LEONARDO® laser system series. The patent pending glass tip of the XCAVATOR® fiber ensures a safe treatment of benign prostate hyperplasia powered by optimized absorption in water and hemoglobin.



- Unique glass tip makes the XCAVATOR® as the first choice treating prostate glands from small to quite large
- Increased contact surface area results in a wider area of tissue resection
- Efficient vaporization, coagulation and resection
- Specially designed resectoscope decreases likelihood of costly optic damage
- Optimized field of view due to vapor bubbles concentrated at fiber tip only
- Tissue resection with possible histological diagnosis
- Short learning curve

TWISTER

The new TWISTER XL fiber is designed to increase the well known ablation rates of the TWISTER L and improve precision fiber handling by optimizing rigidity. Larger fiber tip design increases the surface area to almost 20 % larger than the TWISTER L. A specially designed coating enhances the rigidity and handling of the fiber tip while increasing durability.




- Increased fiber tip surface area for fast and efficient ablation
- Contact mode for tactile feedback
- Increased control of the fiber tip
- Excellent hemostasis
- Short catheter time and fast recovery
- Cystoscope compatibility in line with TWISTER L



Several other urological laser applications

efficient – smooth – gentle

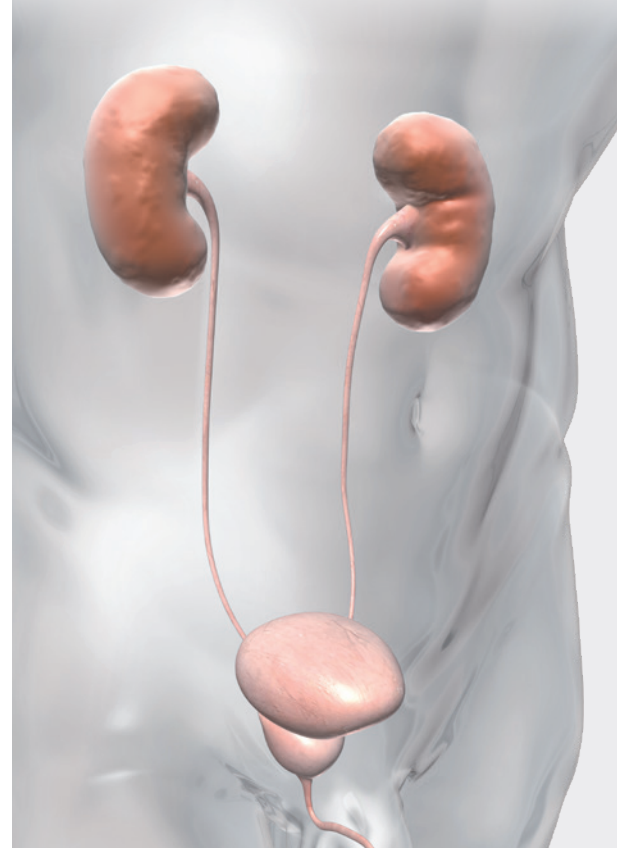


Upper tract tumors

- Comfortable treatment of upper tract tumors with a very thin fiber via a flexible cystoscope
- This avoids an open or laparoscopic surgery
- Fast and minimal invasive surgery


Condyloma

- Smooth and gentle laser condyloma treatment
- Smooth surface after the treatment
- No scars

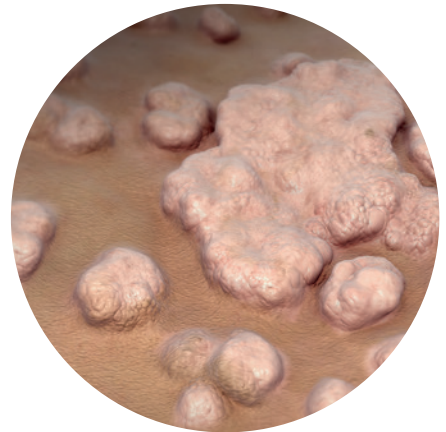

Stricture

- No or very low bleeding
- Always a good view during the procedure
- Easy and comfortable handling

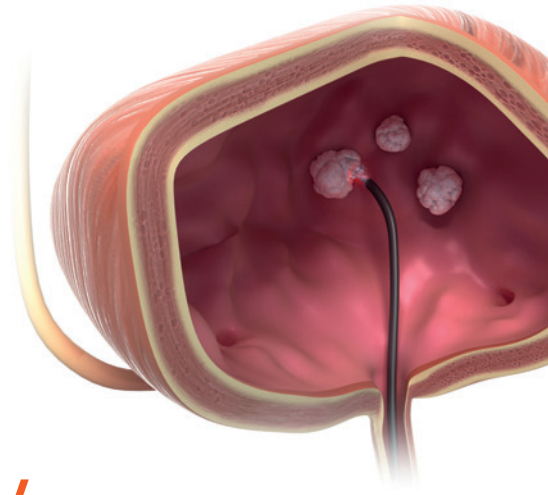


Tumor surgery

Our specialty fibers ensure a safe treatment of bladder tumors powered by optimized absorption in water and hemoglobin when utilizing the LEONARDO® DUAL 200 Watt or LEONARDO® DUAL 45 Watt.

Bladder tumors

The ability of simultaneous cutting and coagulation offers a simple and safe method with a minimal to non loss of blood. Different methods are possible, the standard procedure in an operating room with general/regional anesthesia or outpatient procedure which is even tolerate of high risk patient. The outpatient procedure using a flexible cystoscopy and different kinds of bare fibers does not require general/regional anesthesia and is a gentle way of treating bladder tumors. Both laser treatments for bladder tumors reduce risks for the patient and can be performed quickly.

- Outpatient procedure using flexible cystoscopy
- Tolerated with high risk patient
- Can be performed safely and effectively in the office

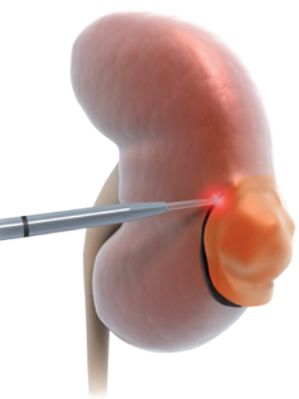

Partial nephrectomy

Cutting and coagulation properties of our optical fibers contribute to a successful nephron sparing surgery securing better overall renal function. Our high-tech fibers would be the fiber of choice to ensure best results. Cutting and coagulating at the same time provides minimal bleeding with a good view on the tissue. Use of our special diode lasers for (open, laparoscopic or robotic) partial nephrectomy offers benefit of no or shorter warm ischemia time with more effective tissue coagulation, hemostasis and reduced parenchymal damage.

- Less bleeding
- No need of suppressing feeding arteries – no time pressure
- Cutting and coagulating at the same time
- Laparoscopic or open procedure




LEONARDO®

| Model | LEONARDO® DUAL 200 | LEONARDO® DUAL 45 |
|------------------------|--|---|
| REF | SL980+1470nm200W | SL980+1470nm45W |
| Wavelength | 980 nm and 1470 nm | 980 nm and 1470 nm |
| Max. power | 200 Watt (1470 nm/40 Watt + 980 nm/160 Watt) individually adjustable | 45 Watt (1470 nm/15 Watt + 980 nm/30 Watt), individually adjustable |
| Fiber diameter | ≥ 360 µm | ≥ 360 µm |
| Aiming beam | 532 nm and 635 nm, green 1 mW, red 4 mW, user-defined intensity | 532 nm and 635 nm, green 1 mW, red 4 mW, user-defined intensity |
| Treatment mode | CW, pulse mode, ELVeS® signal, ELVeS® segment, derma mode | CW, pulse mode, ELVeS® signal, ELVeS® segment, derma mode |
| Pulse duration /-break | 0.01 – CW/0.01 – 60 sec | 0.01 – CW/0.01 – 60 sec |
| Power supply | 110 – 240 VAC, 50/60 Hz, 850 VA | 110 – 240 VAC, 50/60 Hz, 450 VA |
| Dimensions (H×W×D) | approx. 20 cm × 37 cm × 26 cm | approx. 28 cm × 37 cm × 9 cm |
| Weight | approx. 15 kg | approx. 8.5 kg |



| Model | LEONARDO® Mini Dual | LEONARDO® Mini 1470 nm |
|------------------------|--|---|
| REF | SL980+1470nm14W | SL1470nm12W |
| Power / Wavelength | 10 W (980 nm) / 4 W (1470 nm) | 12 W (1470 nm) |
| Fiber diameter | ≥ 360 µm | ≥ 360 µm |
| Aiming beam | 635 nm, max. 4 mW | 635 nm, max. 4 mW |
| Treatment mode | CW, pulse mode (optional) | CW, pulse mode (optional), ELVeS® signal |
| Pulse duration /-break | 0.01 – 180 sec / 0.01 – 180 sec | 0.01 – 180 sec / 0.01 – 180 sec |
| Power supply | 110 – 240 VAC, 50 - 60 Hz (12 VDC @ 65 W) | 110 – 240 VAC, 50 – 60 Hz (12 VDC @ 100 W) |
| Batteries | Li-ion Batteries | Li-ion Batteries |
| Dimensions (H × W × D) | 6 cm × 9 cm × 21.5 cm | 6 cm × 9 cm × 21.5 cm |
| Weight | 900 g | 900 g |

All laser sets comprise 3 safety goggles, foot switch, interlock connector, power cord and manual in a carrying case. The LEONARDO® DUAL 45 Watt is only suitable for the treatment of vesical tumours, partial kidney resection and other low-grade applications with low wattage settings. The standard device in urology primarily used for BPH treatment and all other applications is the LEONARDO® DUAL 200 Watt. The LEONARDO® DUAL 45 is the suitable laser system for partial nephrectomy, bladder tumors, strictures, condylomas etc. The LEONARDO® Mini is the suitable laser system for bladder tumors, strictures, condylomas, etc.

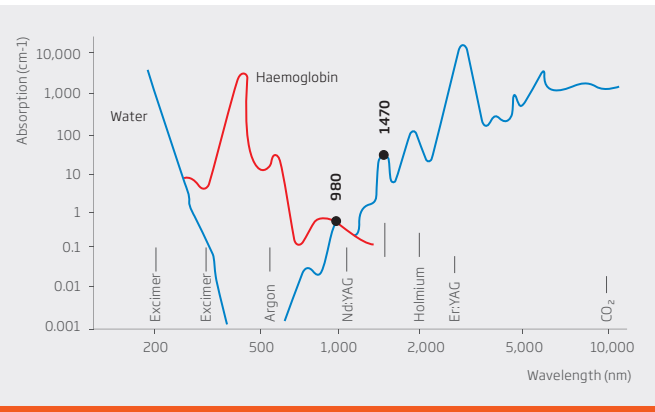

LEONARDO® DUAL 200 Watt – Unique combination of two simultaneous wavelengths

LEONARDO® DUAL 200 Watt combines the wavelengths of 980 nm and 1470 nm with high absorption in H₂O and hemoglobin for multiple applications not only in urology. Wavelength of 980 nm provides high absorption in hemoglobin and is therefore well suited for applications in urology. Due to absorption properties the emitted laser beam does not affect the bladder.

LEONARDO® DUAL 200

VISIBLE LASER RADIATION
AVOID EYE OR SKIN EXPOSURE TO
DIRECT OR INDIRECT RADIATION
CLASS 4 LASER PRODUCT
Diode-Laser 980 +/- 30 nm CW 160 W (Max.)
Diode-Laser 1470 +/- 30 nm CW 40 W (Max.)
IEC 60825-1:2007 IEC 60601-2-22:2007

VISIBLE LASER RADIATION
AVOID EYE EXPOSURE TO DIRECT RADIATION
CLASS 3R LASER PRODUCT
Diode-Laser 635 +/- 10 nm CW 4 mW (Max.) (Aiming)
Diode-Laser 532 +/- 10 nm CW 1 mW (Max.) (Aiming)
IEC 60825-1:2007 IEC 60601-2-22:2007

LEONARDO® DUAL 45

VISIBLE LASER RADIATION
AVOID EYE OR SKIN EXPOSURE TO
DIRECT OR INDIRECT RADIATION
CLASS 4 LASER PRODUCT
Diode-Laser 980 +/- 30 nm CW 30 W (Max.)
Diode-Laser 1470 +/- 30 nm CW 15 W (Max.)
EN 60825-1:2008 EN 60601-2-22:2007

VISIBLE LASER RADIATION
AVOID EYE EXPOSURE TO DIRECT RADIATION
CLASS 3R LASER PRODUCT
Diode-Laser 635 +/- 10 nm CW 4 mW (Max.) (Aiming)
Diode-Laser 532 +/- 10 nm CW 1 mW (Max.) (Aiming)
EN 60825-1:2008 EN 60601-2-22:2007

LEONARDO Mini Dual

VISIBLE LASER RADIATION
AVOID EYE OR SKIN EXPOSURE TO
DIRECT OR INDIRECT RADIATION
CLASS 4 LASER PRODUCT
Diode-Laser 980 +/- 30 nm CW 10 W (Max.)
Diode-Laser 1470 +/- 30 nm CW 4 W (Max.)
IEC 60825-1:2007 IEC 60601-2-22:2007

VISIBLE LASER RADIATION
AVOID EYE EXPOSURE TO DIRECT RADIATION
CLASS 3R LASER PRODUCT
Diode-Laser 635 +/- 10 nm CW 4 mW (Max.) (Aiming)
IEC 60825-1:2007 IEC 60601-2-22:2007

LEONARDO Mini 1470 nm

VISIBLE LASER RADIATION
AVOID EYE OR SKIN EXPOSURE TO
DIRECT OR INDIRECT RADIATION
CLASS 4 LASER PRODUCT
Diode-Laser 1470 +/- 30 nm CW 8 W (Max.)
IEC 60825-1:2007 IEC 60601-2-22:2007

VISIBLE LASER RADIATION
AVOID EYE EXPOSURE TO DIRECT RADIATION
CLASS 3R LASER PRODUCT
Diode-Laser 635 +/- 10 nm CW 4 mW (Max.) (Aiming)
IEC 60825-1:2007 IEC 60601-2-22:2007



CE 1984


CeramOptec GmbH
Siemensstr. 44, D-53121 Bonn



Handpieces and instruments

| REF | Product |
|-----------|---|
| 500400355 | Storz Laser Cystoscope Set (blue) OD 23 Fr ID 7.5 Fr, no optics, incl. external and internal sheath and obturator |
| 400400250 | XCAVATOR® Resectoscope 360° Rotating and Continues Irrigation Set OD 26 Fr, no optics |
| AB2731 | ASAP 30° Optics Hopkins II, compatible Storz Laser Cystoscope blue and XCAVATOR® Resectoscope |
| 400100100 | Universal Dual Luer Handpiece, for ø 600-1000 µm fibers |
| 400400110 | Laparoscopic sheath 30 cm, ID ø 1.4 mm, OD ø 5 mm |
| 400400115 | Laparoscopic sheath 40 cm, ID ø 1.4 mm, OD ø 5 mm |

Fibers for LEONARDO®

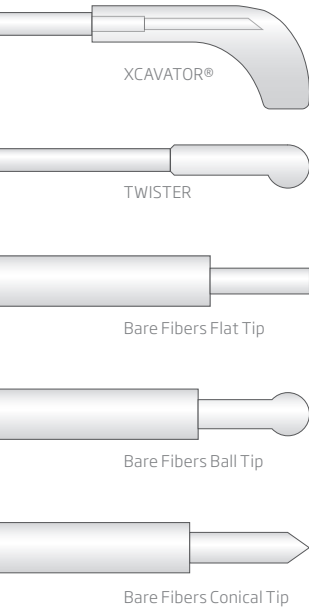

| REF LEONARDO® | Product LEONARDO® | Length [m] | Core ø [Fr] | AD ø [µm]/[Fr] |
|---------------------------|---|------------|-------------|----------------|
| BPH | | | | |
| 503200250 | XCAVATOR® Fiber | 3 | 1.8 | – |
| 503200220 | TWISTER Large Fiber | 3 | 1.8 | 3100/9.3 |
| 503200235 | TWISTER XL Fiber | 3 | 1.8 | 3300/9.3 |
| Other Applications | | | | |
| 503200744 | Bare Fiber 400 µm, Flat Tip, IC | 3 | 400/1.2 | 750/2.3 |
| 503200740 | Bare Fiber 600 µm, Flat Tip, IC | 2.6 | 1.7 | 860/2.6 |
| 503300400 | Bare Fiber 1000 µm, Flat Tip, IC | 2.6 | 2.9 | 1400/4.2 |
| 503200750 | Bare Fiber 600 µm, Ball Tip, Adj. Luer, IC (1 × 6 h) | 2.5 | 1.7 | 860/2.6 |
| 503300410 | Bare Fiber 1000 µm, Ball Tip, IC | 2.6 | 2.9 | 1400/4.2 |
| 503200741 | Bare Fiber 600 µm, Conical Tip, IC | 2.6 | 1.7 | 860/2.6 |
| 503300405 | Bare Fiber 1000 µm, Conical Tip, IC | 2.6 | 2.9 | 1400/4 |
| Enucleation | | | | |
| 503200745 | Bare Fiber 600 µm, Flat Tip, Adj. Luer, ID (1 × 6 h) | 3 | 565/1.7 | 860/2.6 |
| 503300415 | Bare Fiber 1000 µm, Flat Tip, Adj. Luer, ID (1 × 6 h) | 2.6 | 945/2.9 | 1400/4 |


All fibers are free of latex and DEHP. Our fibers are single use products (unless otherwise indicated), delivered sterile for immediate use.

Accessories

| REF | Product |
|-----------|---|
| LA1371 | Laser safety goggles 950 – 110 L4 + 1470 L2 (FULL) type: earpiece |
| LA5199 | Laser safety goggles DIR 804 – 1755 L3 (FULL), type: basket, clear |
| LA5165 | Sticker Laser warning 20 × 20 cm |
| 400100115 | Medi Strip 0.7/1.2 BF 600 µm, autoclavable – Fiber stripper for Bare Fiber 600 µm |
| AB1323 | Stripping tool for fibers 0.3 – 1 mm |
| AB1908 | Touhy Borst adapter |
| AB2594 | Biopsy needle (for the handpiece) |
| 400400200 | Camera Filter HPD 980 nm and 1470 nm, small, OD 24 mm* |

* With high wattages (100 watt) for a good view on the screen

Fibers for holmium laser systems

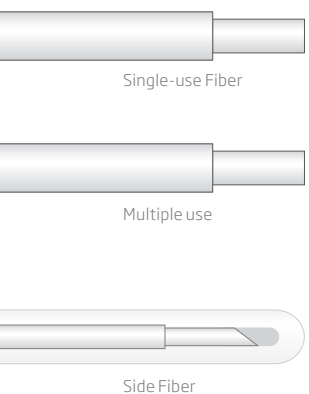


| REF | Product | Length [m] | Core ø [µm]/[Fr] | AD ø [µm]/[Fr] | Connector | NA |
|-------------------------|--------------------------------------|------------|------------------|----------------|-----------|-----------|
| Single-use Fiber | | | | | | |
| 500200326 | Megabeam HBF SF 230 – 253, OD 420 µm | 3.1 | 272 | 420 | SMA905 | 0.28 |
| 500200327 | Megabeam HBF SF 365 – 403, OD 550 µm | 3.1 | 365 | 550 | SMA905 | 0.22/0.37 |
| 500200328 | Megabeam HBF SF 550 – 603, OD 750 µm | 3.1 | 550 | 750 | SMA905 | 0.22/0.37 |
| Multiple use | | | | | | |
| 500200789 | Megabeam RHBFSF 230/253 – 3 | 3.0 | 272 | 420 | SMA905 | 0.22/0.36 |
| 500200790 | Megabeam RHBFSF 365/400 – 3 | 3.0 | 365 | 550 | SMA905 | 0.22/0.36 |
| 500200791 | Megabeam RHBFSF 550/605 – 3 | 3.0 | 550 | 750 | SMA905 | 0.22/0.36 |
| 500200792 | Megabeam RHBFSF 945/1000 – 3 | 3.0 | 945 | 1400 | SMA905 | 0.22/0.36 |
| Side Fiber | | | | | | |
| 500300451 | Megabeam SF – 2100 – H | 3.2 | 550 | 950 | SMA905 | 0.22 |

All fibers are free from latex and DEHP. Our fibers are designed for single use only (unless otherwise indicated), delivered sterile for immediate use. Fibers are compatible with, but not limited to: StoneLight®, COHERENT®, Deka, LUMENIS®, Dornier MedTech and NewStarLasers systems.

Contact us

to learn more about a whole new world
of minimally invasive laser therapies

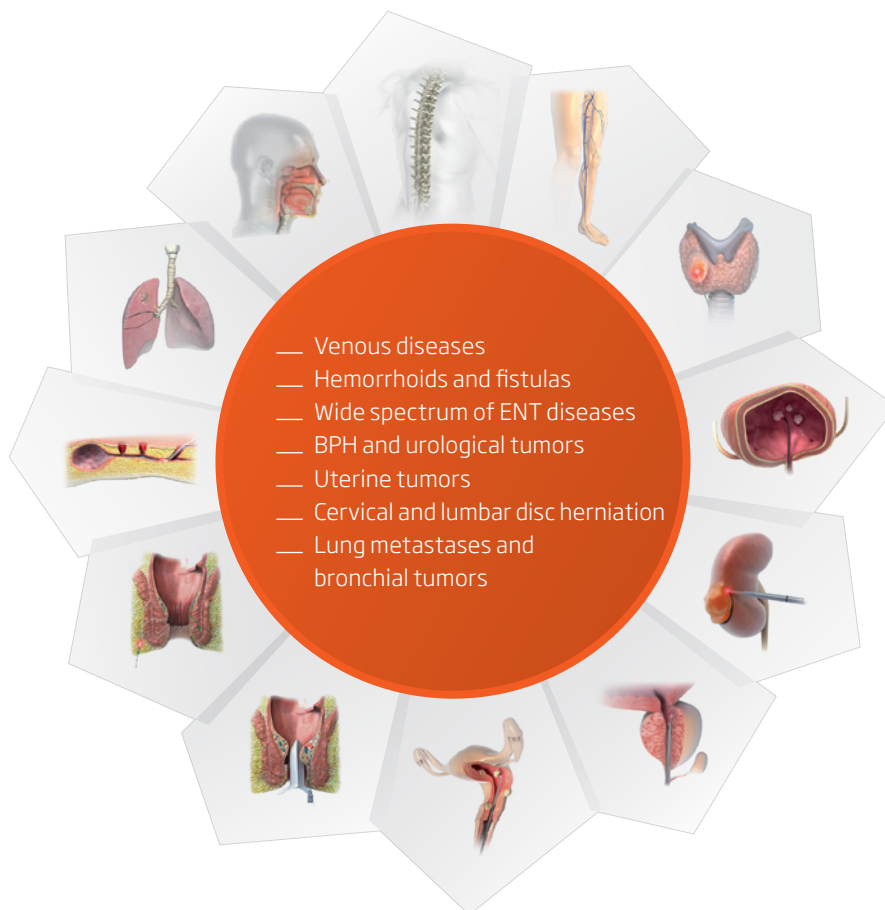

biolitec® worldwide

biolitec Holding GmbH & Co KG

Vienna, Austria
phone: +43 1 3619 909 50
info@biolitec.de
www.biolitec.com

biolitec biomedical technology GmbH

Jena, Germany
Phone: +49 3641 519 53 0

biolitec Schweiz GmbH

Wollerau, Switzerland
Phone: +41 55 555 30 20

biolitec España

Madrid, Spain
Phone: +34 91 9910857

biolitec Italia SRL

Milano, Italy
Phone: +39 02 8423 0633

biolitec Tıbbi Cihazları Ltd. Şti.

Istanbul, Turkey
Phone: +90 216 574 7456

OOO biolitec Spb

Saint-Petersburg, Russia
Phone: +7 812 4493752

biolitec FZ LLC

Dubai, UAE
Phone: +971 44 29 85 92

biolitec laser science and technology Shanghai Ltd.

Shanghai, China
Phone: +86 21 6308 8856

biolitec Sdn. Bhd.

Selangor, Malaysia
Phone: +60 3 5569 7158

biolitec India Private Ltd.

Bangalore, India
Phone: +91 93275 11005

PT. Biolitec

Tangerang, Indonesia
Phone: +62 21 295 57 419

biolitec Korea Ltd.

Seoul, Republic of Korea
Phone: +82 2 701 4707

Equipos Laser de Uso Médico y Fibra Óptica SA de CV

(Biolitec Mexico & Latín América)
Phone: +52 (55) 5573 1800

Biolitec Biotecnologia Comércio, Importação, Exportação LTDA

São Paulo, Brazil
Phone: +55 11 2093 8602

CeramOptec GmbH

Bonn, Germany
Phone: +49 228 979670

Ceram Optec SIA

Rīga, Latvia
Phone: +371 653 25 994



All fibers are free of latex and DEHP. Our fibers are single use products (unless otherwise indicated) delivered sterile for immediate use.

Imprint

biolitec Holding GmbH & Co KG
Untere Viaduktgasse 6/9
A-1030 Wien
Phone: +43 1 3619 909 50
www.biolitec.com